



---

## Product Manual

### **RhD & Rh CcEe Genemer™** **Primer Pair for Gene Specific Fragment Amplification**

Catalog No.: 40-2002-10; 40-2003-10

Store at -20 °C

**For research use only.** Not for use in diagnostic procedures for clinical purposes

---

---

## Material Supplied

---

# RhD & Rh CcEe Genemer™

## Primer Pair for Gene Specific Fragment Amplification

---

### Storage Instructions:

1. Shipped lyophilized at room temperature.
  2. Store at -20 °C upon receipt.
  3. Store at -20 °C after reconstitution.
- 

	Product	Catalog Number	Unit Size
<input type="checkbox"/>	RhD Genemer™ RhD gene specific amplification primer pair	40-2002-10	10 nmole
<input type="checkbox"/>	RhCcEe Genemer™ RhCcEe gene specific amplification primer pair	40-2003-10	10 nmole

---


## RhD & RhCcEe

### Background

The Rh based blood grouping is termed positive or negative based on the presence or absence of the D antigen. Rh allo-immunization in Rh negative pregnant women is of concern because of the potential for the fetus to develop hemolytic disease of newborns and autoimmune diseases. Anemia leading to hydrops, perinatal death, or both occurs in 25% of fetuses sensitized to the RhD antigen in the absence of optimal management. In utero diagnosis and treatment considerably improves the condition with survival rates greater than 75% in severely affected fetuses. However these invasive therapies may be unnecessary in some cases if the fetal Rh status were known prenatally.

A method of determining fetal Rh status early in pregnancy is now possible by DNA analysis of amniotic cells (1). The Rh blood group locus consists of two related structural genes, *D* and *CcEe*. These highly homologous genes which share greater than 96% identity in their coding region have been cloned and the molecular basis of the Rh blood group established (2). The RhD-positive and RhD-negative polymorphism is associated with the presence or the absence of the *D* gene (there is no 'd' gene). The C/c and E/e antigens are encoded by a unique gene. The E/e associated nucleotide polymorphism results in one amino acid substitution at position 226 (proline to alanine), whereas the C/c antigenic polymorphism consists of six nucleotide substitutions leading to four amino acid changes at position 16 (Cys16Trp), 60 (Ile60Leu), 68 (Ser68Asn) and 103 (Ser103Pro).

DNA analysis for Rh genotype loci specifically amplifies DNA fragments for the RhD and RhCcEe gene. Due to the high sensitivity and specificity of the test at the DNA level, occasionally the results may not match those obtained by serologic methods. The test will type individuals as RhD positive who are D<sup>u</sup> low grade status serologically (3-5), this is due to the absence of the gene product at the protein level due to partial deletions. The total error rate should be less than 1%.

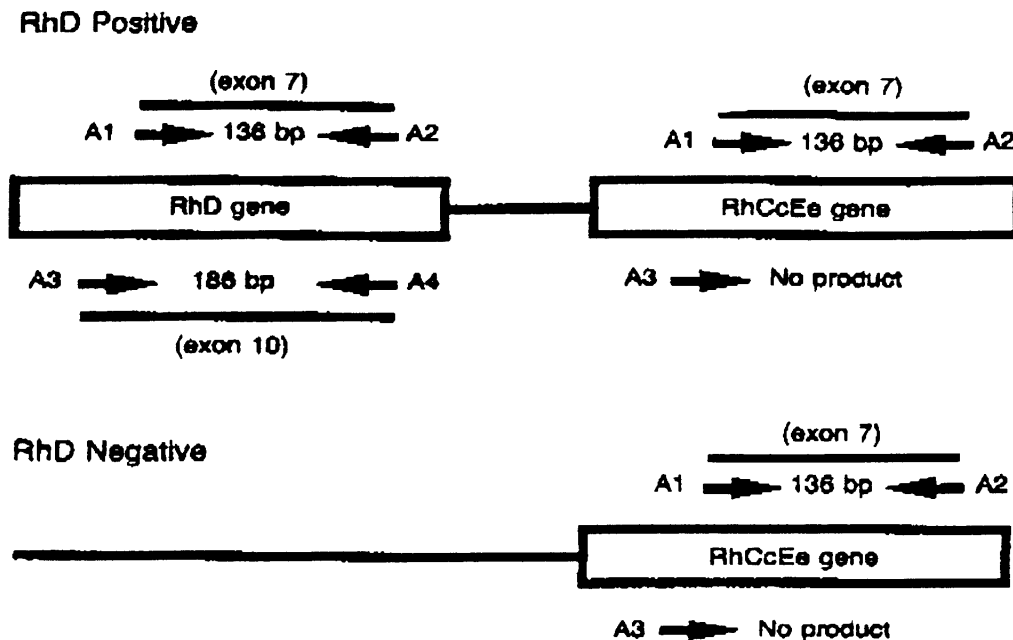

## Procedure

### Material Supplied

Each tube supplied contains the lyophilized primer Genemer™ pair. Please refer to label on the specific tube. Each tube contains 10 nmols. The quantity supplied is sufficient for 400 regular 50 µl PCR reaction.

#### A. Genemer™ Reconstitution

**Stock Primer Mix:** Dissolve the supplied lyophilized Genemer™ in 100 µl sterile TE. The 10 nmols of primers when dissolved in 100 µl will give a solution of 100 µM i.e. 100 pmols/µl.

**Primer Mix:** Prepare a 10 pmols/µl Primer Mix solution by a ten fold dilution of the stock primer mix. Example: Add 180 µl sterile TE to a new tube, to this tube add 20 µl of primer stock solution. Label this tube as Primer Mix 10 pmols/µl.

#### B. Thermal Cycler Files Amplification Profile

The following amplification profile has been optimized for specific product amplification using the supplied Genemer™.

Program the following thermal cycler files.

##### 1. Hot Start

Rh Hot Start		
Step	Time & Temperature	Cycles
Initial Denaturation	95 °C for 5 minutes	1
Annealing	50 °C Hold Infinity	Hold
Comments: Add Taq premix while on hold.		

##### 2. Amplification File

Rh Amplification File			
Step	Temperature	Time	Cycles
Denaturation	94 °C	30 sec.	30
Annealing	52 °C	30 sec.	
Elongation	72 °C	1 minute	
Fill in Extension	72 °C	7 minutes	1
Hold	4 °C	Infinity	Hold

#### C. PCR

##### 1. PCR Premix Preparation (PP). Label tube "PP"

PCR Premix Preparation (PP)		
Component	1 X 50 µl Rxn.	10 X 50 µl Rxns.
Sterile Water	32 µl	320 µl
10 X PCR Buffer	4.5 µl	45 µl
2.0 mM dNTP	5 µl	50 µl
10 pmol/µl Primer Mix	2.5 µl	25 µl
Template DNA (~500 ng)	1-2 µl	Add DNA to each tube
Total Volume	45 µl	
After adding template start hot start PCR File		

Dispense 44 µl of the above PCR premix to individual PCR tubes for each amplification reaction and then add the template DNA. Start "Hot Start" thermal cycler file. While holding at 50 °C add 5 µl of the Taq Enzyme Mix (EM). Start amplification file.

##### 2. Taq Polymerase mix Preparation (EM). Label tube "EM"

### RhD & CcEeGenemer™ [40-2002-10] Amplification of specific Rh Fragments

For research use only. Not for use in diagnostic procedures for clinical purposes.

Taq Enzyme Mix Preparation (EM)		
Component	1 X 50 µl Rxn.	10 X 50 µl Rxns.
Sterile Water	5 µl	50 µl
10 X PCR Buffer	0.5 µl	5 µl
Taq Polymerase	0.5 µl	5 µl
Add 5 µl to each reaction when holding after hot start		

#### D. Agarose Electrophoresis

Load 10 to 15 µl samples to 1.8% agarose gel. Run at 90 mAmps. Confirm correct amplification fragment size.

## Results and Interpretation

Genemer™ specific for RhD gene exon 10 (Catalog No. 40-2002-10) will amplify a 186 bp fragment specific and Genemer™ specific for RhCcEe gene exon 7 (Catalog No. 40-2003-10) will amplify a 136 bp fragment as shown in the figure below. Multiplex can be performed.

Normal PCR amplified fragment size		
Genemer™	RhD Genotype	RhCcEe Genotype
RhCeEe	136 bp	136 bp
RhD	186 bp	None
Multiplex RhCeEe & RhD	136 & 186 bp	Only 136 bp

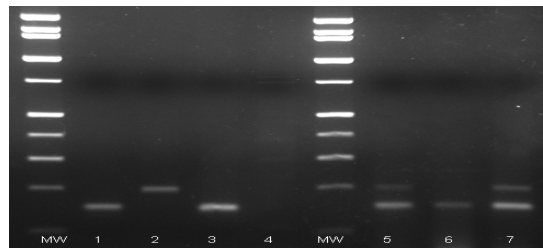


Figure. MW lanes are molecular weight markers. Lanes 1,2, 5 & 7 represent PCR from a Rh D positive DNA and Lanes 3,4 & 6 represent PCR from Rh D negative DNA. Lanes 1 & 3 PCR product of RhCcEe Genemer™ amplification, lanes 2 & 4 from RhD Genemer™ amplification. Lane 5, 6 & 7 represent multiplex amplification of RhCcEe and RhD.

## References

1. Bennet, P.R., et al. (1993) Prenatal determination of fetal RhD type by DNA amplification. NEJM 329:607-610.
2. Mouro, I., et al. (1993) Molecular genetic basis of the human Rhesus blood group system. Nature Genetics 5:62-65.
3. Simsek, S., Bleeker, P.M., Borne, A. E.G. (1994) Prenatal determination of fetal RhD type. NEJM 330:795.
4. Bennet, P., Warwick, R. and Carton, J-P. (1994) Prenatal determination of fetal RhD type. NEJM 330:795-796.
- Westhoff, C.M. and Wylie, D.E. (1994) Identification of a new RhD-specific mRNA from K562 cells. Blood 84:3098-3100

## Appendix

### Genomic DNA Purification

Genomic DNA is usually extracted from blood. A simple procedure is given below that purifies ~10 µg DNA from 300 µl blood using a 30 minute procedure.

Omni-Pure™ Genomic DNA Purification System  
Rapid DNA Purification Protocol for 300 µl Whole Blood

Catalog Number: 40-4010-01

#### A. Initial Preparation

1. Label two sets of eppendorf tubes per sample.
2. Add 900 µl GD-1 solution (RBC Lysis Solution) to one tube for each sample.
3. Add 300 µl Isopropanol (2-propanol) to one tube for each sample. Cap the tubes.

#### B. Cell Lysis

1. To the tube containing 900 µl GD-1 solution (RBC Lysis Solution) using a filter tip pipet transfer 300 µl whole blood. Cap and gently mix by inversion. Incubate for 1-3 minutes at room temperature. Mix by inversion a few times during this incubation period. Incubate longer for fresh blood cells as they are intact and not lysed already.
2. Centrifuge at 3 K rpm for 20 seconds to pellet the white blood cells. A reddish white pellet should be clearly visible. Decant and discard supernatant leaving behind the last few droplets. Do not totally remove the supernatant.
3. Completely resuspend the white blood cell pellet by vigorously vortexing the tube. Ensure that the pellet is completely resuspended.
4. To the resuspended cells add 300 µl GD-2 solution (Cell Lysis Solution). Mix by gentle vortexing. You will notice release of DNA by the thickening of the liquid in the sample. Samples may be stored at this stage for processing later. It has been shown that the samples are stable in Cell Lysis Solution for at least 2 years at room temperature.

#### C. Protein Precipitation

1. Add 100 µl GD-3 solution (Protein Precipitation Solution) to the sample in cell lysis solution.
2. Vortex vigorously at for 20 seconds. Small particles of brown color will be appear and be visible at this stage.
3. Centrifuge at 5 K rpm for 1 minute to pellet the precipitated proteins. A clearly visible brown pellet containing proteins should be collected at the bottom of the tube.

#### D. DNA Precipitation

1. Decant the supernatant containing the DNA to a new appropriately labeled tube (see initial preparation above) containing 300 µl 100% Isopropanol (2-propanol).
2. Mix the sample by inversion till a visible white floating DNA strand-particle is identified. 30-40 mixing by inversion is usually sufficient.
3. Centrifuge at 6 K rpm for 1 minute to collect the DNA as a pellet. A white DNA pellet should be clearly visible.
4. Decant supernatant and place tube inverted on a clean Kimwipe™ tissue paper to drain the remaining supernatant.
5. To remove residual salts, add 300 µl of 70% ethanol. Vortex gently.
6. Centrifuge at 6 K rpm for 1 minute to collect the DNA as a pellet. Gently take out the tubes so that the pellet is not dislodged. While holding the tube, rotate tube so that you can watch the pellet. Now carefully decant the ethanol, keeping an eye on the pellet so that it does not flow away.
7. Place tube inverted on a clean Kimwipe™ tissue paper to drain the remaining ethanol.
8. Air dry the DNA pellet. Do not use vacuum.

#### E. DNA Reconstitution & Use

1. Add 100 µl of GD-4 solution (DNA Reconstitution Solution). Vortex gently. Incubate at 60°C for 5 minutes to facilitate dissolution or keep overnight at room temperature.
2. Store DNA at 4°C. For long-term storage, place sample at -20°C or -80°C.
3. Average yield of 10 µg is expected from 300 µl blood DNA. The range is between 5 µg to 15 µg.
4. The 100 µl of purified DNA obtained will have an average concentration of ~ 100 ng/µl.
5. For PCR amplification use 1-2µl.
6. Use 100 µl for restriction digestion followed by Southern blot analysis.
7. It is convenient to perform multiple 300 µl blood DNA purification instead of scaling up the procedure.

## PCR Components and Analysis

### Buffer Condition

PCR buffer conditions vary and it is imperative to optimize buffer conditions for each amplification reaction. At Gene Link most amplification reactions have been optimized to work with the following standard buffer condition, unless indicated.

Standard Gene Link PCR Buffer Composition	
10 X PCR buffer	1 X PCR buffer
100 mM Tris-HCl pH 8.3	10 mM
500 mM KCl	50 mM
15 mM MgCl <sub>2</sub>	1.5 mM
0.01% Gelatin	0.001%

### dNTP Concentration

Standard dNTP concentration of 0.2mM of each base is used. See section on PCR additives when dNTP concentration is changed.

Recipe	
2.0 mM dNTP Stock Solution Preparation*	
Component	Volume
100 mM dGTP	100 µl
100 mM dATP	100 µl
100 mM dTTP	100 µl
100 mM dCTP	100 µl
Water	4.6 ml
<b>Total Volume</b>	<b>5 ml</b>
*Aliquot and freeze	

### MgCl<sub>2</sub> Concentration

The concentration of Mg<sup>++</sup> will vary from 1-5 mM, depending upon primers and substrate. Since Mg<sup>2+</sup> ions form complexes with dNTPs, primers and DNA templates, the optimal concentration of MgCl<sub>2</sub> has to be selected for each experiment. Low Mg<sup>2+</sup> ions result in a low yield of PCR product, and high concentrations increase the yield of non-specific products and promote mis-incorporation. Lower Mg<sup>2+</sup> concentrations are desirable when fidelity of DNA synthesis is critical. The recommended range of MgCl<sub>2</sub> concentration is 1-4 mM, under the standard reaction conditions specified. At Gene Link, using the standard PCR buffer with KCl, a final dNTP concentration of 0.2 mM, a MgCl<sub>2</sub> concentration of 1.5 is used in most cases. If the DNA samples contain EDTA or other chelators, the MgCl<sub>2</sub> concentration in the reaction mixture should be raised proportionally. Given below is an MgCl<sub>2</sub> concentration calculation and addition table using a stock solution of 25 mM MgCl<sub>2</sub>.

MgCl <sub>2</sub> Concentration & Addition Table								
Final concentration of MgCl <sub>2</sub> in 50µl reaction mix, (mM)	1.0	1.25	1.5	1.75	2.0	2.5	3.0	4.0
Volume of 25mM MgCl <sub>2</sub> , µl	2	2.5	3	3.5	4	5	6	8

### Primer Concentration

The final concentration of primers in a PCR reaction is usually 0.5 to 1 µM (micromolar). This is equivalent to 0.5 to 1 pmol/µl. For a 100 µl reaction you would add 50 to 100 pmols. At Gene Link we use 0.5 pmol/µl in the final PCR.

### Genemer™ Reconstitution

**Stock Primer Mix:** Dissolve the supplied 10 nmols of lyophilized Genemer™ in 100 µl sterile TE. The 10 nmols of primers when dissolved in 100 µl will give a solution of 100 µM i.e. 100 pmols/µl.

For research use only. Not for use in diagnostic procedures for clinical purposes.

**Primer Mix:** Prepare a 10 pmols/μl Primer Mix solution by a ten fold dilution of the stock primer mix.

Example: Add 180 μl sterile TE to a new tube, to this tube add 20 μl of primer stock solution. Label this tube as Primer Mix 10 pmols/μl.

### Amplification Thermal Cycling

**Hot Start:** It is essential to have a 'Hot Start' profile for amplification of any fragment from a complex template like human genomic DNA. Taq polymerase has low activity at room temperature and it is essential to minimize any mis-priming in the first cycle of amplification. A typical hot start profile is given below. Various enzyme preparations are available which are activated by heat in the first cycle. A simple hot start protocol is given below that can be used with regular Taq polymerase. See the section on PCR additives for amplification of products from high GC content templates.

Hot Start		
Step	Time & Temperature	Cycles
Initial Denaturation	95 °C for 5 minutes	1
Annealing	60 °C Hold Infinity	Hold
Comments: Add Taq premix while on hold.		

### Amplification File

The initial denaturation step at 94 °C for 30 seconds is sufficient for all templates. The number of cycles is usually set to 30 and is sufficient to amplify 1-10 μg of product depending on the initial concentration of template. A higher number of cycles from 35-45 cycles may be used, but internal priming on the product and over amplification of unwanted bands often result from over-cycling. Generally, it is better to focus on optimizing reaction conditions than to go beyond 35 cycles.

Typical Amplification File			
Step	Temperature	Time	Cycles
Denaturation	94 °C	30 sec.	30
Annealing	*	30 sec.	
Elongation	72 °C	30 sec.	
Fill in Extension	72 °C	7 minutes	1
Hold	4 °C	Infinity	Hold
Based on the T <sub>m</sub> of the primers. Usually varies from 50°C to 65°C			



**Typical Reaction Premix**

Typical PCR Premix (/50µl)	
Component	Volume
10 x PCR Buffer	5 µl
2.0 mM dNTP mix (each)	5 µl
Primer Mix (10 pmol/µl each) or 2.5µl of 10 pmol/µl of individual primer (final 25 pmol of each primer/50µl)	2.5 µl
H <sub>2</sub> O	37.5 µl
<b>Total Volume</b>	<b>50 µl</b>

**Typical PCR Reaction Mix**

PCR reaction (/50µl)	
Component	Volume
PCR premix	45 µl
100ng/µl diluted DNA	1 µl
Hot start and then add	
Taq premix	5 µl


**Taq Premix Preparation**

Taq Premix (/50µl)	
Component	Volume
PCR Premix	6 µl
Taq polymerase (5 u/µl)	0.25µl
<b>Add 5µl/50 µl rxn. After initial denaturation</b>	
Use 2.5 units of Taq for 100 µl reactions. Taq is usually supplied at a concentration of 5 units/µl	

**Yield and Kinetics**

The target will be amplified by up to 10<sup>6</sup> fold in a successful reaction, but the amplification will usually plateau at 1-10µg. Thus, 1 pg of target sequence in the reaction is a good place to begin.

PCR reactions produce product in a nonlinear pattern. Amplification follows a typical exponential curve until some saturation point is reached. Generally products will not be further amplified once 1-5 µg has been generated. Saturation by one product of a reaction does not always prevent further amplification of other generally unwanted products. Over-cycling may decrease the quality of an otherwise good reaction. When first optimizing a reaction, it is advisable to take samples every 5 or 10 cycles to determine the number of cycles actually needed.



## Gel Electrophoresis of PCR Products

Gel electrophoresis of PCR products is the standard method for analyzing reaction quality and yield. PCR products can range up to 10kb in length, but the majority of amplifications are at 1kb and below. Agarose electrophoresis is the classical method to analyze amplification products from 150 bp to greater than 10kb. Polyacrylamide gel electrophoresis should be used for resolution of short fragments in the range of 100 bp to 500 bp when discrimination of 10 bp difference is required.

PAGE gels for PCR products formulated with the amount of cross-linker chosen to give pore sizes optimal for the size of DNA fragment desired. Gels are most often stained in ethidium bromide, even though the fluorescence of this stain is quenched by polyacrylamide, which decreases sensitivity 2-5 fold. This decrease in sensitivity generally does not present a problem, because most PCR reactions yield product levels in the microgram range, and Ethidium will detect as little as 1/10 of this amount. Polyacrylamide gels can be stained by silver staining for more sensitive detection.

## Purification of PCR Product

Various purification methods are available for the purification of PCR products. The selection of a particular method over other is based on the downstream application and the initial robustness of the amplification. Usually no further purification is required for most cloning experiments if a single fragment is amplified, whereas for sequencing application the amplified product should be purified from the primers and any other minor amplification products.

The preferred method of purification of an amplified fragment is the excision of the fragment band after agarose gel electrophoresis. This method yields the purification of a single fragment; as such care should be taken to excise a gel piece containing a single electrophoretically resolved fragment. Omni-Clean™ Purification System available from Gene Link can be used for this purpose. Catalog No. **40-4110-10 for bead based system; 40-4120-10 for spin column based system and 40-4130-10 for DNA concentration. Please refer to product insert for detailed protocol or visit [www.genelink.com](http://www.genelink.com)**

- A. **Purification of DNA from gel slices using glass beads. Provides purified single fragment.**  
[Omni-Clean™ Gel DNA Beads Purification System; Catalog No. 40-4110-10]

### Protocol

1. By weight, determine the volume of the excised DNA fragment.
2. Add 3 volumes of NaI solution and heat to 55°C. Visually determine the dissolution of gel pieces.
3. Add 1 µl of glass bead suspension per µg of DNA and vortex.
4. Centrifuge at 2K rpm for 20 seconds to pellet glass bead/DNA complex. Discard supernatant.
5. Re-suspend pellet in 400 µl Omni-Clean™ wash buffer. Centrifuge at 2K rpm for 20 seconds and discard wash buffer.
6. Pipet out any remaining buffer in the tube.
7. Add 25 µl water or TE; re-suspend pellet and centrifuge at 2K rpm for 20 seconds.
8. The supernatant contains the purified DNA. Using a pipet, collect the supernatant and transfer to a new appropriately labeled tube.

- B. **Purification of DNA from gel slices using spin column. Provides purified single fragment.**  
[Omni-Clean™ Gel DNA Spin Column Purification System; Catalog No. 40-4120-50]

### Protocol

1. By weight, determine the volume of the excised DNA fragment.
2. Add 3 volumes of NaI solution and heat to 55°C. Visually determine the dissolution of gel pieces.
3. Add the above solution to the spin column assembled on a collection tube.
4. Let the solution flow by gravity or centrifuge at 2K rpm for 20 seconds. Discard flow through collected in the collection tube.
5. Add 400 µl Omni-Clean™ wash buffer to the spin column. Centrifuge at 2K rpm for 2 minutes and discard wash buffer collected in the collection tube.
6. Replace the collection tube with a new appropriately labeled eppendorf tube.
7. Add 25 µl water or TE to the spin column. Let sit for 3 minutes.
8. Centrifuge at 2K rpm for 2 minutes.
9. The collection tube contains the purified DNA.

- C. **Purification of DNA from solution using glass beads. Provides removal of salts, primers and dNTP.** [Omni-Clean™ DNA Beads Concentration System; Catalog No. 40-4130-10]

**Protocol**

1. Determine volume of DNA solution and add 3 volumes of NaI solution.
2. Add 1 µl of glass bead suspension per µg of DNA.
3. Centrifuge at 2K rpm for 20 seconds to pellet glass bead/DNA complex. Discard supernatant.
4. Re-suspend pellet in 400 µl Omni-Clean™ wash buffer.
5. Centrifuge at 2K rpm for 20 seconds and discard wash buffer.
6. Pipet out any remaining buffer in the tube.
7. Add 25 µl water or TE; re-suspend pellet and centrifuge at 2K rpm for 20 seconds.
8. The supernatant contains the purified DNA. Using a pipet, collect the supernatant and transfer to a new appropriately labeled tube.

**D. Purification of DNA from solution using spin column. Provides removal of salts, primers and dNTP.** [Omni-Clean™ DNA Spin Column Concentration System; Catalog No. 40-4140-10]**Protocol**

1. Determine volume of DNA solution and add 3 volumes of NaI solution.
2. Add the above solution to the spin column assembled on a collection tube.
3. Let the solution flow by gravity or centrifuge at 2K rpm for 20 seconds. Discard flow through collected in the collection tube.
4. Add 400 µl Omni-Clean™ wash buffer to the spin column. Centrifuge at 2K rpm for 2 minutes and discard wash buffer collected in the collection tube.
5. Replace the collection tube with a new appropriately labeled eppendorf tube.
6. Add 25 µl water or TE to the spin column. Let sit for 3 minutes.
7. Centrifuge at 2K rpm for 2 minutes.
8. The collection tube contains the purified DNA.

**PEG Precipitation**

Primers and salts are efficiently removed by a simple PEG precipitation. This method is recommended for downstream DNA sequencing application. This method is generally used for plasmid DNA.

**Protocol**

1. To 50 µl of amplified PCR reaction add 6.0 µl of 5 M NaCl and 40 µl of 13% (w/v) PEG 8000. Incubate the mixture on ice for 20-30 minutes.
2. Collect the DNA precipitate by centrifugation at maximum speed for 15 minutes at 4°C in a microfuge. Carefully remove the supernatant by gentle aspiration.  
*The pellet of DNA is translucent and generally invisible at this stage.*
3. Rinse the pellet with 500 µl of 70% ethanol.  
The precipitate changes to a milky-white color and becomes visible.
4. Carefully pour off the 70% ethanol. Rinse the DNA pellet once more with 70% ethanol. Store the tube in an inverted position at room temperature until the last visible traces of ethanol have evaporated.
5. Dissolve the DNA in 20µl of H<sub>2</sub>O.
6. Run an aliquot on an agarose gel to confirm the presence of the correct amplified product. The purified DNA is sequence grade and can be used directly for sequencing.

**Gel Filtration**

Primers and salts are efficiently removed by gel filtration using Sephadex G-50. This method is recommended for downstream DNA sequencing application.

**Protocol**

1. Hydrate Sephadex G-50 ahead of time in sterile water or TE (10mM Tris pH 8, 1 mM EDTA). Take out from fridge if already stored hydrated. Bring to room temperature.
2. Assemble a spin column on a collection tube.
3. Add 700µl of hydrated Sephadex G-50 to each spin column, initiate flow using rubber bulb or any other method.
4. Allow flowing by gravity till there is no more fluid left above the Sephadex G-50 bed. Discard flow through from the collection tube.
5. Spin the spin column placed inside the collection tube for 2 minutes at 3 K rpm.
6. Change collection tube to new 1.5 ml eppendorf tube appropriately labeled with sample name.
7. Apply up to 50 µl sample gently to the G-50 bed of the column.
8. Spin for 2 minutes at 3 K rpm.
9. Purified sample is collected in the collection tube. The eluent collected in the 1.5 ml eppendorf tube is free of salts and primers shorter than 35-40mer.

### PCR Additives

DNA polymerases need to elongate rapidly and accurately to function effectively *in vivo* and *in vitro*, yet certain DNA regions appear to interfere with their progress. One common problem is pause sites, at which DNA polymerase molecules cease elongation for varying lengths of time. Many strong DNA polymerase pauses are at the beginnings of regions of strong secondary structure such as template hairpins (1). Taq polymerase use in PCR suffers the same fate and GC-rich DNA sequences often require laborious work to optimize the amplification assay. The GC-rich sequences possess high thermal and structural stability, presumably because the high duplex melting temperature that permits stable secondary structures to form, thus preventing completion of a faithful replication (2).

Nucleotide analog 7-deaza dGTP is effective in reducing the secondary structure associated with GC rich region by reducing the duplex stability(4). Betaine, DMSO and formamide reduces the  $T_m$  and the complex secondary structure thus the duplex stability (1-5). Tetramethyl ammonium chloride (TMAC) actually increases the specificity of hybridization and increases the  $T_m$ . The use of TMAC is recommended in PCR conditions using degenerate primers.

These PCR additives and enhancing agents have been used to increase the yield, specificity and consistency of PCR reactions. These additives may have beneficial effects on some amplification and it is impossible to predict which agents will be useful in a particular context and therefore they must be empirically tested for each combination of template and primers.

PCR Additives		
Additive	Purpose & Function	Concentration
7-deaza-2'-deoxyguanosine; 7-deaza dGTP	GC rich region amplification. Reduce the stability of duplex DNA	Totally replace dGTP with 7-deaza dGTP; or use 7-deaza dGTP: dGTP at 3:1
Betaine (N,N,N-trimethylglycine = [carboxymethyl]trimethylammonium)	Reduces T <sub>m</sub> facilitating GC rich region amplification. Reduces duplex stability	Use 3.5M to 0.1M betaine. Be sure to use Betaine or Betaine (mono)hydrate and <b>not</b> Betaine HCl.
BSA (bovine serum albumin)	BSA has proven particularly useful when attempting to amplify ancient DNA or templates which contain PCR inhibitors such as melanin.	BSA concentration of 0.01µg/µl to 0.1µg/ µl can be used.
DMSO (dimethyl sulfoxide)	DMSO is thought to reduce secondary structure and is particularly useful for GC rich templates.	DMSO at 2-10% may be necessary for amplification of some templates, however 10% DMSO can reduce <i>Taq</i> polymerase activity by up to 50% so it should not be used routinely.
Formamide	Reduces secondary structure and is particularly useful for GC rich templates.	Formamide is generally used at 1-5%. Do not exceed 10%.
Non-ionic detergents e.g. Triton X-100, Tween 20 or Nonidet P-40 (NP-40)	Non-ionic detergents stabilise <i>Taq</i> polymerase and may also suppress the formation of secondary structure.	0.1-1% Triton X-100, Tween 20 or NP-40 may increase yield but may also increase non-specific amplification. As little as 0.01% SDS contamination of the template DNA (left-over from the extraction procedure) can inhibit PCR by reducing <i>Taq</i> polymerase activity to as low as 10%, however, inclusion of 0.5% Tween-20 or -40 will effectively neutralize this effect.
TMAC (tetramethylammonium chloride)	TMAC is used to reduce potential DNA-RNA mismatch and improve the stringency of hybridization reactions. It increases T <sub>m</sub> and minimizes mis-pairing.	TMAC is generally used at a final concentration of 15-100mM to eliminate non-specific priming.

**References:**

1. Kovarova, M; and Draber, P; (2000) New Specificity and yield enhancer for polymerase chain reactions (2000) Nucl. Acids. Res. 28: e70.
2. Henke, W., Herdel, K., Jung, K., Schnorr, D. and Stefan A. Loening, S. (1997) Betaine improves the PCR amplification of GC-rich DNA sequences. Nucl. Acids Res. 25: 3957-3958.
3. Daniel S. Mytelka, D.S., and Chamberlin, M.J.,(1996) Analysis and suppression of DNA polymerase pauses associated with a trinucleotide consensus. Nuc. Acids Res.,. 24:2774-278.
4. Keith, J. M., Cochran, D.A.E., Lala, G.H., Adams, P., Bryant, D. and Mitchelson, K.R. (2004) Unlocking hidden genomic sequence. Nucl. Acids Res. 32: e35.
5. Owczarzy, R., Dunietz, I., Behlke, M.A., Klotz, I.M. and Joseph A. Walder. (2003) Thermodynamic treatment of oligonucleotide duplex-simplex equilibria. PNAS, 100:14840-14845.

## Genemer™ Product Ordering Information

Genemer™ Primer pair for gene or mutation specific amplification. Special optimized conditions may be required for certain amplifications

Product	Size	Catalog No.
Fragile X (spanning CGG triple repeat region) Genemer™; 10 nmols	10 nmols	40-2004-10
Huntington Disease (spanning CAG triple repeat region) Genemer™; 10 nmols	10 nmols	40-2025-10
Myotonic Dystrophy (spanning CTG triple repeat region) Genemer™; 10 nmols	10 nmols	40-2026-10
Friedreich's Ataxia (spanning GAA triple repeat region) Genemer™; 10 nmols	10 nmols	40-2027-10
Factor V Genemer™; 10 nmols	10 nmols	40-2035-10
Factor VIII (Hemophilia) Genemer™ Pack Genemer™; 10 nmols	10 nmols	40-2036-10
STS (Steroid Sulfatase) Genemer™; 10 nmols	10 nmols	40-2023-10
HGH (Human Growth Hormone) Genemer™; 10 nmols	10 nmols	40-2024-10
Sickle Cell Genemer™; 10 nmols	10 nmols	40-2001-10
RhD (Rh D gene exon 10 specific) Genemer™; 10 nmols	10 nmols	40-2002-10
Rh EeCc (Rh Ee and Cc exon 7 specific) Genemer™; 10 nmols	10 nmols	40-2003-10
Gaucher (various mutations) Genemer™; 10 nmols	10 nmols	40-2047-XX
Cystic Fibrosis (various mutations) Genemer™; 10 nmols	10 nmols	40-2029-XX
SRY (sex determining region on Y) Genemer™; 10 nmols	10 nmols	40-2020-10
X alphoid repeat Genemer™; 10 nmols	10 nmols	40-2021-10
Y alphoid repeat Genemer™; 10 nmols	10 nmols	40-2022-10

## Genemer™ Control DNA Product Ordering Information

Genemer™ control DNA is a cloned fragment of the mutation region of a particular gene. These control DNA are an ideal genotyping template for optimizing and performing control amplification with unknown DNA.

Product	Size	Catalog No.
Sickle Cell Genemer control DNA (HbA, S and C available)	500 ng	40-2001-0X
GLFX CGG Genemer Control DNA; Fragile X (16, 29, 40, 60 & 90 CGG repeats available)	500 ng	40-2004-0X
GLHD CAG Genemer Control DNA; Huntington Disease (18, 34, 44, 89 & 134 CAG repeats available)	500 ng	40-2025-0X
GLDM CTG Genemer Control DNA; Myotonic Dystrophy (12, 45, 93, 129 & 194 CTG repeats available)	500 ng	40-2026-0X

## GeneProber™ Product Ordering Information

The GeneProber™ product line is based on the chemiluminescent Southern blot detection method. Gene Link's non-radioactive detection systems for genotyping of triple repeat disorders are rapid, reliable and as sensitive as the <sup>32</sup>P labeled southern blots. No more decayed probes and radioactive exposure. Kits are available for reliable genotyping of the fragile X, myotonic dystrophy and other triple repeat mutation group disorders.

**Unlabeled GeneProber™ probes are also available for radio labeling and radioactive based detection.** Gene Link strongly recommends the use of non-radioactive gene detection systems. Consider switching to Gene Link's product line of non-radioactive detection systems

Product	Size	Catalog No.
Fragile X GeneProber™ GLFX1 Probe unlabeled	500 ng	40-2004-40
Fragile X GeneProber™ GLFXDig1 Probe Digoxigenin labeled	110 µL	40-2004-41
Huntington's Disease GeneProber™ GLHD14 Probe unlabeled	500 ng	40-2025-40
Huntington's Disease GeneProber™ GLHDDig2X Probe Digoxigenin labeled	110 µL	40-2025-41
Myotonic Dystrophy GeneProber™ GLDM1 Probe unlabeled	500 ng	40-2026-40
Myotonic Dystrophy GeneProber™ GLDMDig2 Probe Digoxigenin labeled	110 µL	40-2026-41
Friedreich's Ataxia GeneProber™ GLFRDA21 Probe unlabeled	500 ng	40-2027-40
Friedreich's Ataxia GeneProber™ GLFRDADig21 Probe Digoxigenin labeled	110 µL	40-2027-41

## GScan™ Products Product Ordering Information

Gene Link's GScan™ gene detection products are safe, convenient and sensitive, and afford automated compilation of data. The kits contain optimized PCR amplification reagents and a wide array of fluorescent-labeled primers for genotyping after PCR using fluorescent genetic analyzer instrument(s). Included in these kits are ready-to-run control samples of various repeats of the triple repeat disorder kit. These control samples are for calibration with the molecular weight markers for accurate size determination of the amplified fragments.

The GScan™ kits are simple and robust for routine triple-repeat detection of greater than 100 repeats of all triple repeat disorders listed, except Fragile X. The CGG repeat in Fragile X can be detected up to ~50 repeats.

Product	Size	Catalog No.
Fragile X GScan™ Kit for fluorescent detection; 100 reactions kit	1 kit	40-2004-15XX
Fragile X GScan™ Kit for fluorescent detection; 20 reactions kit	1 kit	40-2004-15FMS
Huntington's Disease GScan™ Kit for fluorescent detection; 100 reactions kit	1 kit	40-2025-15XX
Huntington's Disease GScan™ Kit for fluorescent detection; 20 reactions kit	1 kit	40-2025-15FMS
Myotonic Dystrophy GScan™ Kit for fluorescent detection; 100 reactions kit	1 kit	40-2026-15XX
Myotonic Dystrophy GScan™ Kit for fluorescent detection; 20 reactions kit	1 kit	40-2026-15FMS
Friedreich's Ataxia GScan™ Kit for fluorescent detection; 100 reactions kit	1 kit	40-2027-15XX
Friedreich's Ataxia GScan™ Kit for fluorescent detection; 20 reactions kit	1 kit	40-2027-15FMS

All Gene Link products are for research use only

Current pricing are posted at <http://www.genelink.com/>

## Related Products Ordering Information

**Omni-Pure™ DNA & RNA Purification Systems**

Product	Catalog No.	Unit Size*(Purifications)
Omni-Pure™ Blood DNA Purification System	40-4010-01	100
Omni-Pure™ Blood DNA Purification System	40-4010-05	500
Omni-Pure™ Blood DNA Purification System	40-4010-10	1000
Omni-Pure™ Tissue DNA Purification System	40-4050-01	100
Omni-Pure™ Tissue DNA Purification System	40-4050-05	500
Omni-Pure™ Tissue DNA Purification System	40-4050-10	1000
Omni-Pure™ Plant DNA Purification System	40-4060-01	100
Omni-Pure™ Plant DNA Purification System	40-4060-05	500
Omni-Pure™ Plant DNA Purification System	40-4060-10	1000
Omni-Pure™ Viral DNA Purification System	40-3720-01	100
Omni-Pure™ Viral DNA Purification System	40-3720-05	500
Omni-Pure™ Microbial DNA Purification System	40-3700-01	100
Omni-Pure™ Microbial DNA Purification System	40-3700-05	500
Omni-Pure™ Viral RNA Purification System	40-3650-01	100
Omni-Pure™ Viral RNA Purification System	40-3650-05	500

\*Sample volume for each purification system varies. Each purification yields sufficient quantity for desired applications.

**Omni-Clean™ Gel DNA Purification and Concentration Systems**

Product	Catalog No.	Unit Size*(Purifications)
Omni-Clean™ Gel DNA Beads Purification System	40-4110-10	100
Omni-Clean™ Gel DNA Beads Purification System	40-4110-50	500
Omni-Clean™ Gel DNA Spin Column Purification System	40-4120-10	100
Omni-Clean™ Gel DNA Spin Column Purification System	40-4120-50	500
Omni-Clean™ DNA Beads Concentration System	40-4130-10	100
Omni-Clean™ DNA Beads Concentration System	40-4130-50	500
Omni-Clean™ DNA Spin Column Concentration System	40-4140-10	100
Omni-Clean™ DNA Spin Column Concentration System	40-4140-50	500

\*Sample volume for each purification system varies. Each purification yields sufficient quantity for desired applications.

**Omni-Pure™ Plasmid DNA Purification Systems**

Product	Catalog No.	Unit Size*(Purifications)
Omni-Pure™ Plasmid DNA Purification System	40-4020-01	100
Omni-Pure™ Plasmid DNA Purification System	40-4020-05	500

\*Sample volume for each purification system varies. Each purification yields sufficient quantity for desired applications.

All Gene Link products are for research use only

Current pricing are posted at <http://www.genelink.com/>



## Related Products Ordering Information

### Taq Polymerase & Master Mix

Product	Catalog No.	Unit Size
Taq DNA Polymerase; 400 units; 5 µL; 80 µL	40-5200-40	400 units
Taq PCR Kit; 200 x 50 µL reactions	40-5211-01	200 reactions
Taq PCR Kit with controls; 200 reactions	40-5212-01	200 reactions
PCR Master Mix (2X); 100 x 50 µL reactions (2 tubes x 1.3 mL)	40-5213-01	100 reactions
PCR Master Mix (2X); 200 x 50 µL reactions (4 tubes x 1.3 mL)	40-5213-02	200 reactions

## Related Products Ordering Information

### PCR Additives & Reagents

Product	Catalog No.	Unit Size
Taq DNA Polymerase 300 units; 5 µL; 60 µL	40-5200-30	300 units
PCR Buffer Standard (10 X); 1.6 mL	40-3060-16	1.6 mL
PCR Buffer Mg Free (10 X) ; 1.6 mL	40-3061-16	1.6 mL
Taq Polymerase Dilution Buffer; 1 mL	40-3070-10	1 mL
dNTP 2mM (10X) ; 1.1 mL	40-3021-11	1.1 mL
MgCl <sub>2</sub> ; 25 mM; 1.6 mL	40-3022-16	1.6 mL
Omni-Marker™ Universal Unlabeled; 100 µL	40-3005-01	100 µL
Primer and Template Mix; 500 bp; 40 reactions; 100 µL	40-2026-60PT	100 µL
Nuclease Free Water; 1.6 mL	40-3001-16	1.6 mL
DMSO; 1 mL	40-3031-10	1 mL
TMAC (Tetramethyl ammonium chloride) 100 mM; ; 1 mL	40-3053-10	1 mL
KCl 300 mM; 1 mL	40-3059-10	1 mL
Betaine; 5M; 1 mL	40-3032-10	1 mL

### Omni-Marker™

Product	Catalog No.	Unit Size*
Omni-Marker™ Universal unlabeled; 100 µL	40-3005-01	100 µL
Omni- Marker™ Universal unlabeled; 500 µL	40-3005-05	500 µL
Omni-Marker™ Universal unlabeled; 1 mL	40-3005-10	1 mL
Omni- Marker™ Low unlabeled; 100 µL	40-3006-01	100 µL
Omni-Marker™ Low unlabeled; 500 µL	40-3006-05	500 µL
Omni- Marker™ Low unlabeled; 1 mL	40-3006-10	1 mL
Omni-Marker™ GScan-2 Tamra labeled 50 bp - 600 bp; 100 µL	40-3062-01	100 µL
Omni-Marker™ GScan-2 Tamra labeled 50 bp - 600 bp; 500 µL	40-3062-05	500 µL

All Gene Link products are for research use only

Current pricing are posted at <http://www.genelink.com/>

## Southern Blot Buffers & Reagents

Product	Catalog No.	Unit Size
Agarose Tablets, 0.5 gm each 100 Tablets	40-3011-10	100 tablets
Agarose LE Molecular Biology Grade; 100 g	40-3010-10	100 g
Agarose LE Molecular Biology Grade; 500 g	40-3010-50	500 g
Hybwash A, Hybridization Wash Solution; 200 mL	40-5020-20	200 mL
Hybwash B, Hybridization Wash Solution; 100 mL	40-5021-10	100 mL
TAE Buffer; 50X Concentrate; 100 mL	40-3007-01	100 mL
TAE Buffer; 50X Concentrate; 1 L	40-3007-10	1 L
TBE Buffer; 5X Concentrate; 1 L	40-3008-10	1 L
10x Washing buffer; 200 mL	40-5025-20	200 mL
10% Blocking solution; 100 mL	40-5026-10	100 mL
Seq. Loading buffer; 1 mL	40-5027-00	1 mL
10x AP Detection buffer; 100 mL	40-5031-10	100 mL
Lumisol™ I Hybridization Solution; contains formamide; 200 mL	40-5022-20	200 mL
Lumisol™ II Hybridization Solution; for non-toxic hybridizations; 200 mL	40-5023-20	200 mL
Lumisol™ III Hybridization Solution; for oligo probes; 200 mL	40-5024-20	200 mL

## Loading Buffers

Product	Catalog No.	Size
Gel Loading Buffer 5X BPB/XC non-denaturing; 1 mL	40-3002-10	1 mL
Gel Loading Buffer 5X BPB/XC non-denaturing; 15 mL	40-3002-15	15 mL
Gel Loading Buffer 10X BPB/XC non-denaturing; 1 mL	40-3003-10	1 mL
Gel Loading Buffer 10X BPB/XC non-denaturing; 15 mL	40-3003-15	15 mL
Gel Loading Buffer 5X Orange G/XC non-denaturing; 1 mL	40-3004-10	1 mL
Gel Loading Buffer 5X Orange G/XC non-denaturing; 15 mL	40-3004-15	15 mL
Gel Loading Buffer 2X BPB/XC Denaturing for Sequencing; 1 mL	40-5027-10	1 mL
Gel Loading Buffer 2X BPB/XC Denaturing for Sequencing; 15 mL	40-5027-15	15 mL
DNA SDS Gel Loading Buffer 5X BPB/XC DNA binding protein denaturing buffer; 1 mL	40-5028-10	1 mL
DNA SDS Gel Loading Buffer 5X BPB/XC DNA binding protein denaturing buffer; 15 mL	40-5028-15	15 mL
RNA Gel Loading Buffer 2X BPB/XC with ethidium bromide; 1 mL	40-5029-10	1 mL
RNA Gel Loading Buffer 2X BPB/XC with ethidium bromide; 15 mL	40-5029-15	15 mL
RNA Gel Loading Buffer 2X BPB/XC without ethidium bromide; 1 mL	40-5030-10	1 mL
RNA Gel Loading Buffer 2X BPB/XC without ethidium bromide; 15 mL	40-5030-15	15 mL

All Gene Link products are for research use only

Current pricing are posted at <http://www.genelink.com/>

